

RESEARCH

Open Access

Myocardial T_1 and T_2 mapping at 3 T: reference values, influencing factors and implications

Florian von Knobelsdorff-Brenkenhoff^{1,2*}, Marcel Prothmann^{1,2}, Matthias A Dieringer^{1,2}, Ralf Wassmuth^{1,2}, Andreas Greiser³, Carsten Schwenke⁴, Thoralf Niendorf^{1,5} and Jeanette Schulz-Menger^{1,2}

Abstract

Background: Myocardial T_1 and T_2 mapping using cardiovascular magnetic resonance (CMR) are promising to improve tissue characterization and early disease detection. This study aimed at analyzing the feasibility of T_1 and T_2 mapping at 3 T and providing reference values.

Methods: Sixty healthy volunteers (30 males/females, each 20 from 20–39 years, 40–59 years, 60–80 years) underwent left-ventricular T_1 and T_2 mapping in 3 short-axis slices at 3 T. For T_2 mapping, 3 single-shot steady-state free precession (SSFP) images with different T_2 preparation times were acquired. For T_1 mapping, modified Look-Locker inversion recovery technique with 11 single shot SSFP images was used before and after injection of gadolinium contrast. T_1 and T_2 relaxation times were quantified for each slice and each myocardial segment.

Results: Mean T_2 and T_1 (pre-/post-contrast) times were: 44.1 ms/1157.1 ms/427.3 ms (base), 45.1 ms/1158.7 ms/411.2 ms (middle), 46.9 ms/1180.6 ms/399.7 ms (apex). T_2 and pre-contrast T_1 increased from base to apex, post-contrast T_1 decreased. Relevant inter-subject variability was apparent (scatter factor 1.08/1.05/1.11 for T_2 /pre-contrast T_1 /post-contrast T_1). T_2 and post-contrast T_1 were influenced by heart rate ($p < 0.0001$, $p = 0.0020$), pre-contrast T_1 by age ($p < 0.0001$). Inter- and intra-observer agreement of T_2 ($r = 0.95$; $r = 0.95$) and T_1 ($r = 0.91$; $r = 0.93$) were high. T_2 maps: 97.7% of all segments were diagnostic and 2.3% were excluded (susceptibility artifact). T_1 maps (pre-/post-contrast): 91.6%/93.9% were diagnostic, 8.4%/6.1% were excluded (predominantly susceptibility artifact 7.7%/3.2%).

Conclusions: Myocardial T_2 and T_1 reference values for the specific CMR setting are provided. The diagnostic impact of the high inter-subject variability of T_2 and T_1 relaxation times requires further investigation.

Keywords: Cardiovascular magnetic resonance, Heart, T_1 , T_2 , Mapping, 3 T

Background

Cardiovascular magnetic resonance (CMR) provides techniques for non-invasive myocardial tissue characterization. T_1 and T_2 mapping of the left ventricular myocardium, i.e. quantification of the myocardial T_1 and T_2 relaxation times, as well as the T_1 -derived extracellular volume fraction have been demonstrated to add valuable information [1-6]. Most of the experience with myocardial

mapping was gained at a magnetic field strength of 1.5 T. Parametric myocardial mapping at 3 T is conceptually appealing due to the signal gain inherent to higher fields, which may be exploited for improved spatial and temporal resolution [7]. Many of the previous studies focused on intra-individual comparison of diseased and remote myocardium. However, T_2 and T_1 reference values of all myocardial segments may be important to define small focal abnormalities and to identify diffuse tissue changes in the absence of healthy “remote” myocardium. For all these reasons this study scrutinizes myocardial T_1 and T_2 at 3 T in a large sample of healthy volunteers using state-of-the-art mapping techniques.

* Correspondence: florian.von-knobelsdorff@charite.de

¹Berlin Ultrahigh Field Facility, Max-Delbrueck Center for Molecular Medicine, Berlin, Germany

²Working Group on Cardiovascular Magnetic Resonance, Experimental and Clinical Research Center a joint cooperation between the Charité Medical Faculty and the Max-Delbrueck Center for Molecular Medicine HELIOS Klinikum Berlin Buch, Department of Cardiology and Nephrology, Lindenberger Weg 80, 13125, Berlin, Germany

Full list of author information is available at the end of the article

Methods

Study population

60 healthy volunteers were enrolled into the study (30 men/30 women, equally distributed within 3 age categories (Table 1)). The status “healthy” was based on: i) uneventful medical history, ii) absence of any symptoms indicating cardiovascular dysfunction, iii) normal ECG, iv) normal cardiac dimensions and function proven by cine CMR. v) normal myocardial tissue assessed by late enhancement (LGE). For each volunteer written informed consent was obtained prior to the study, after due approval by the ethical committee of the Charité Medical Faculty (EA2/077/10). All experiments were performed in compliance with the Helsinki Declaration.

CMR examination

All CMR exams were performed with a 3 T system (Magnetom Verio, Siemens Healthcare, Erlangen, Germany) using a 32-channel cardiac RF coil for signal reception, the integrated body RF coil for transmission, and ECG for cardiac gating. Subject-specific, volume-selective first- and second-order B_0 -shimming based on field maps derived from double-gradient-echo acquisitions was performed to improve static field uniformity. The following CMR protocols were used (Figure 1).

Cine imaging

Steady-state free-precession (SSFP) cine images were obtained during repeated breath-holds in three long axes (horizontal, vertical, and 3-chamber) and in a stack of

short axes (SAX) covering the left ventricle (LV) to assess wall motion and for cardiac chamber quantification. Imaging parameters were: repetition time (TR) 3.1 ms, echo time (TE) 1.3 ms, asymmetric echo with factor 0.29, flip angle (FA) 45°, field of view (FOV) (276 × 340) mm², matrix 156 × 192, slice thickness 6 mm, receiver bandwidth (BW) 704Hz/px, parallel imaging using GRAPPA reconstruction (R = 2), 30 cardiac phases.

T₂ mapping


For T₂ mapping, data were acquired in basal, mid-ventricular, and apical SAX planes using a T₂-prepared single-shot SSFP technique similar to the one described for 1.5 T [2]. For the application on a 3 T platform, the RF pulse length of the SSFP readout module was increased to reduce the SAR deposition and adiabatic T₂ preparation pulses were employed to improve the homogeneity of the T₂ weighting. Three SSFP images, each with different T₂ preparation time (TE_{T2P} = 0 ms, 24 ms, 55 ms) were acquired in end-diastole within one breath-hold. Imaging parameters were: TR = 2.4 ms, TE = 1 ms, FA = 70°, FOV = (340 × 278) mm², matrix = 176 × 144, slice thickness = 6 mm, BW = 1093Hz/px, GRAPPA acceleration factor 2, linear phase encoding scheme. To correct for residual cardiac and respiratory motion between image sets, a non-rigid registration algorithm was used [8]. A pixel-wise myocardial T₂-map was generated using unsupervised curve-fitting based on a two-parameter equation [2]. The single shot SSFP readout and use of only three TE_{T2P} was chosen to balance accuracy and acquisition time (7 heart cycles) [2,9].

T₁ mapping

For T₁ mapping, data were acquired in basal, mid-ventricular, and apical SAX planes before and 10 - minutes after administration of 0.2 mmol/kg i.v. gadobutrol (Gadovist®, Bayer Healthcare Germany). Data were obtained in end-diastole using a cardiac-gated, SSFP-based Modified Look-Locker Inversion Recovery (MOLLI) technique [10]. For the application at 3 T, the RF pulse length of the SSFP readout module was increased to reduce the SAR deposition. Imaging parameters were: TR = 2.6-2.7 ms, TE = 1.0-1.1 ms, FA = 35°, FOV = (270 × 360)mm², matrix = 156 × 208 to 168 × 224, slice thickness = 6 mm, BW = 1045-1028Hz/px, GRAPPA acceleration factor 2, linear phase-encoding ordering, minimum TI of 91 ms. To generate a pixel-wise myocardial T₁-map, single-shot SSFP images were acquired at different inversion times (pattern 3-3-5, [10]) and registered [8] prior to a non-linear least-square curve fitting using $S(TI) = A - B \exp(-TI/T1^*)$ with $T1 = T1 \times (B/A - 1)$, where A, B, and T1* are estimated by a three parameter fit [11]. In-plane voxel dimensions were kept isotropic to

Table 1 Characteristics of the volunteers

Parameter	Result
Number	60
Females/Males	30/30
Age [years]	48 ± 17
Age group 20–39 years	20 (10 Males/10 Females)
Age group 40–59 years	20 (10 Males/10 Females)
Age group 60–80 years	20 (10 Males/10 Females)
Height [cm]	173 ± 9
Weight [kg]	76 ± 14
Body mass index [kg/m ²]	25 ± 4
Body surface area [m ²]	1.9 ± 0.2
Systolic blood pressure [mm/Hg]	132 ± 12
Diastolic blood pressure [mm/Hg]	72 ± 11
Heart rate [min ⁻¹]	70 ± 6
LV enddiastolic volume [ml]	143 ± 35
LV enddiastolic volume index [ml/cm]	0.8 ± 0.2
LV ejection fraction [%]	64 ± 5
LV mass [mg]	101 ± 26
LV mass index [mg/cm]	0.6 ± 0.2

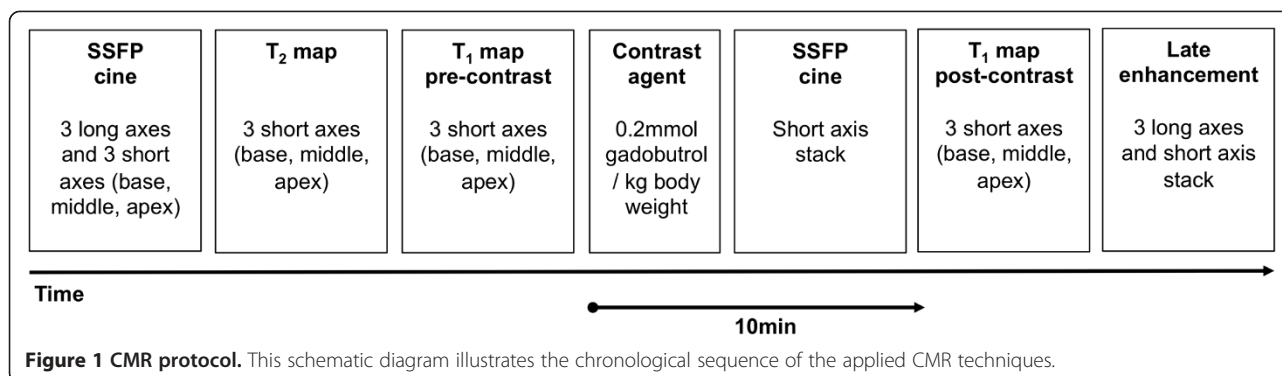

ensure that partial volume effects are independent of slice rotation.

LGE imaging

LGE imaging was performed in the same planes as SSFP CINE imaging using a segmented inversion-recovery gradient-echo sequence beginning 15 minutes after contrast administration. The inversion time (TI) was repeatedly adjusted to appropriately null the myocardium during the length of LGE image acquisition. Imaging parameters were: TR = 10.5 ms, TE = 5.4 ms, FA = 30°, FOV (350 × 262) mm², matrix 256 × 162, slice thickness 6 mm, BW 140Hz/px, GRAPPA acceleration factor 2.

CMR image analysis

Image analysis was done using CMR⁴² (Circle Cardiovascular Imaging, Calgary, Canada).

LV chamber quantification

SSFP cine images were visually evaluated regarding wall motion abnormalities. LV enddiastolic and endsystolic volume and LV mass were determined by manually contouring the endocardial and epicardial borders of the SAX in systole and diastole.

LGE assessment

The absence of LGE was determined qualitatively by visual assessment.

T₂ and T₁ mapping - qualitative assessment

Each single original image was assessed regarding artifacts caused by susceptibility effects, cardiac or respiratory motion. Each motion-corrected series was evaluated whether the images were correctly aligned. Each map was evaluated whether the original images were transformed to a reasonably appearing map. The presence of artifacts led to the exclusion of all affected myocardial segments. Two experienced readers assessed quality in consensus.

T₂ mapping - quantitative assessment

The LV myocardium was delineated by manually contouring the endocardial and epicardial border. We ensured that the region of interest (ROI) was definitely within the myocardium and did not include blood or epicardial fat based. An endocardial and epicardial contour was drawn in one original motion-corrected image. The trabeculated layer and the epicardial border were left out. In doubt, SSFP cine images were consulted. The contours were copied to the other images and adapted to fit in all of these. These final contours were copied to the map. The myocardial ROI was automatically segmented according to the AHA segment model [12]. Results are presented both per segment and averaged per slice.

T₁ mapping - quantitative assessment

T₁ values were recorded from pre-contrast and post-contrast T₁ maps applying the same procedure as for T₂.

T₂ and T₁ mapping - Observer dependency

Intra- and interobserver variability were tested in a subgroup of 20 randomly selected subjects (320 myocardial segments), where one observer measured T₂ and pre-contrast T₁ values of each LV segment twice with at least 3 months of time between the measurements. A second observer measured T₂ and pre-contrast T₁ values blinded to the other results.

Statistical analysis

Baseline characteristics are shown as means with standard deviation (SD) or absolute frequencies. Relaxation times are displayed as least-square means with 95% tolerance intervals (90% coverage) and were assessed by slice and by segment using mixed linear models on logarithmic transformed data to ensure normal distributed data. The following co-factors were included into each model to assess their impact on the relaxation times: age (categories), gender, heart rate (binary with split at median), blood pressure and excluded backwards if not significant. For T₁ and T₂, the scatter factor was

provided as back transformed SD, which allows a similar interpretation as the coefficient of variation for non-transformed data. All values presented were back transformed using the exponential to present the data on the original scale. Spearman's correlation coefficients were calculated to evaluate correlations between the co-factors, which may interfere with the modelling. A p-value of less than 0.05 was regarded as statistically significant. Calculations were performed using SAS 9.2 (SAS Institute Inc., Cary, NC, USA). Intra- and inter-observer dependency was assessed by Bland-Altman analysis and Pearson's correlation using Prism 5.0 (Graphpad Software, La Jolla, CA, USA).

Results

CMR

All 60 CMR scans were performed without major adverse events. The scans were incomplete in 4 subjects. T₂ maps were available for 58 subjects, pre-contrast T₁ maps for 59 subjects and post-contrast T₁ maps for 57 subjects.

T₂ mapping

From 922 segments, 901 (97.7%) were eligible for analysis (Figure 2). A full set of original data and corresponding maps is available as additional file (see Additional file 1). Twenty-one segments (2.3%) were

excluded due to a susceptibility artifact (Figures 2 and 3) mainly in the inferior/inferolateral wall (18 out of 21; 85.7%). Exclusion of at least one segment affected 12 out of 58 subjects (20.7%).

T₂ relaxation times per slice are shown in Table 2. Mean value was 44.1 ms (base), 45.1 ms (middle) and 46.9 ms (apex). All slices differed significantly ($p < 0.0001$) with increasing values from base to apex.

T₂ values for each myocardial segment are presented in Figure 4. Significant segment-to-segment differences were observed in the basal slice ($p = 0.0036$) with slightly lower values in the anterior wall compared to inferior. No significant segment-to-segment differences were found for the midventricular ($p = 0.5398$) and apical slices ($p = 0.1367$). The distribution of all individual T₂ results is illustrated in Figure 5. A relevant inter-subject variability was evident as indicated by a scatter factor of 1.08 (Figure 5 and Table 2).

Heart rate (ranging from 47 to 102 min⁻¹) was found to significantly influence T₂ measurements ($p < 0.0001$). A heart rate higher than the median (69.5 min⁻¹) was associated with lower T₂ values (base: 42.8 ms vs. 45.8 ms; middle: 43.9 ms vs. 46.5 ms; apex: 45.7 ms vs. 48.2 ms). Other tested cofactors including age and gender were not found to be significant.


Pre-contrast T₁ mapping

For pre-contrast T₁ mapping 938 segments were obtained. 859 (91.6%) were eligible for analysis (Figure 2). A full set of original data and corresponding maps is available as additional file (see Additional file 2). Seventy-two segments (7.7%) were excluded due to a susceptibility artifact and 7 segments (0.7%) due to incorrect motion correction (Figures 2, 6 and 7). In 63 out of 72 segments (87.5%) with susceptibility artifact, the inferior/inferolateral segments were affected. Exclusion of at least one segment affected 34 out of 59 subjects (57.6%).

T₁ relaxation times per slice are shown in Table 2. Mean value was 1157.1 ms (base), 1158.7 ms (middle) and 1180.6 ms (apex). Apical T₁ relaxation times were significantly larger than basal and midventricular (each $p < 0.0001$).

T₁ values for each myocardial segment are shown in Figure 4. A significant segment-to-segment difference was found for each slice (basal: $p < 0.0001$; mid: $p < 0.0001$; apex: $p = 0.0153$). T₁ of the anterior segment was lower than in the other segments. The distribution of all individual T₁ results is illustrated in Figure 5. A relevant inter-subject variability was found with a scatter factor of 1.05 (Figure 5, Table 2).

The age categories were found to significantly influence myocardial T₁ relaxation times ($p < 0.0001$). The difference was small between age category 20–39 years

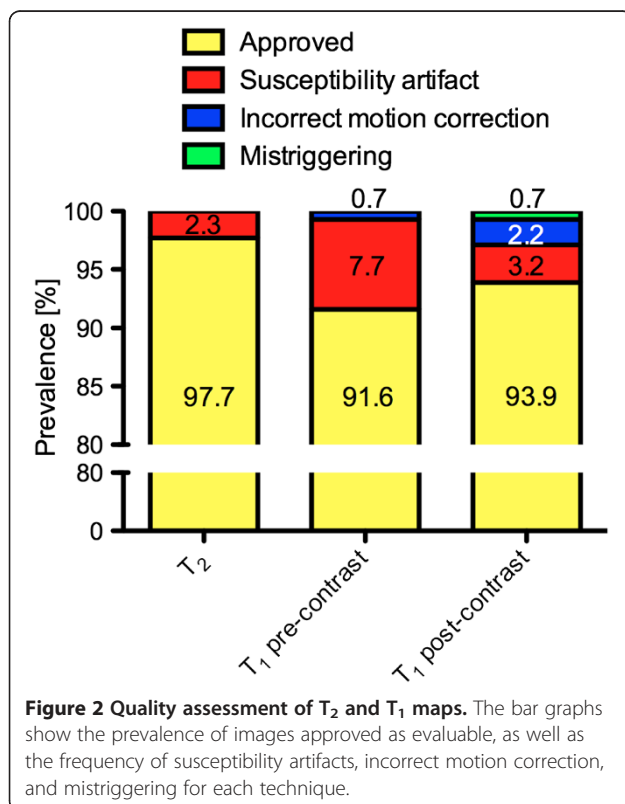

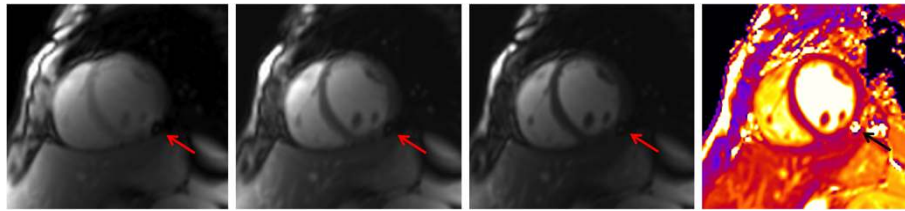


Figure 3 T₂ mapping artifact. Susceptibility artifact in the inferolateral wall of the midventricular plane (red arrow; the 3 grayscale images represent the T₂-prepared SSFP images with different T₂ preparation times). In the map (right image), the artifact is visible in the same area (black arrow).

and 40–59 years. A clear decrease of T₁ relaxation times was observed for subjects ≥ 60 years (Figure 8). Other tested cofactors including heart rate and gender were not found to be significant.

Post-contrast T₁ mapping

For post-contrast T₁ mapping 841 out of 896 segments (93.9%) were eligible for analysis (Figure 2). Twenty-nine segments (3.2%) were excluded due to a susceptibility artifact, which mainly affected the inferior/inferolateral segments (25 out of 29; 86.2%). Six segments (0.7%) were excluded due to mistriggerring (all in one subject). Motion correction failed in one subject in all planes and in one subject in the apical plane leading to an exclusion of 20 segments (2.2%). Exclusion of at least one segment affected 18 out of 56 subjects (32.1%).

T₁ relaxation times per slice are shown in Table 2. Mean values of 427.3 ms (base), 411.2 ms (middle) and 399.7 ms (apex) were obtained. All slices differed significantly from each other (base vs. middle: $p < 0.0001$; base vs. apex $p < 0.0001$; middle vs. apex: $p = 0.0013$) with decreasing T₁ values from base to apex.

T₁ values for each myocardial segment are shown in Figure 4. No significant segment-to-segment differences were observed for each slice (basal: $p = 0.4918$; mid: $p = 0.4741$; apex: $p = 0.5629$). The distribution of all individual T₁ results is illustrated in Figure 5. Post-contrast T₁-maps revealed a relevant inter-

subject variability reflected by a scatter factor of 1.11 (Figure 5, Table 2).

Heart rate was found to significantly influence the post-contrast T₁ relaxation time ($p = 0.0020$) with higher heart rates than the median (69.5 bpm) being associated with lower post-contrast T₁ relaxation times (base: 445.7 ms vs. 418.7 ms; middle: 430.1 ms vs. 405.3 ms; apex: 427.6 ms vs. 388.0 ms). Other tested cofactors including age and gender were not found to be significant.


For T₂ and pre-contrast T₁ mapping inter- and intra-observer analysis demonstrated close agreement (Table 3).

Discussion

This study examined myocardial T₁ and T₂ mapping techniques at 3 T in a large sample of healthy volunteers. The main findings are: i) T₂ and T₁ mapping achieve a high grade of diagnostic image quality, although susceptibility artifacts entailed the exclusion of a limited number of myocardial segments from the analysis. ii) Observer dependency of T₂ and T₁ relaxation time quantification was low. iii) Mean values and 95% tolerance interval of myocardial T₂ and T₁ relaxation times are presented per slice and per segment and can be used as reference values specific for this MR setting. iii) An inter-subject distribution of T₂ and T₁ values became apparent and may constitute a limitation to define appropriate cut-offs.

Table 2 Myocardial T₂ and T₁ relaxation times [in ms] for each plane (base, middle, apex)

	Position	Least square mean	95% Tolerance interval	Min-Max
T ₂ [ms]	Base	44.1	39.3 – 49.5	36.2 – 53.3
	Middle	45.1	39.9 – 50.1	37.9 – 57.0
	Apex	46.9	40.8 – 53.8	39.1 – 59.1
T ₁ pre-contrast [ms]	Base	1157.1	1074.5 – 1246.0	965.6 – 1340.8
	Middle	1158.7	1074.0 – 1250.1	1005.3 – 1295.9
	Apex	1180.6	1073.9 – 1297.9	1106.3 – 1393.9
T ₁ post-contrast [ms]	Base	427.3	363.2 – 502.7	284.5 – 520.1
	Middle	411.2	349.9 – 483.2	282.5 – 513.2
	Apex	399.7	323.0 – 494.6	260.6 – 519.5

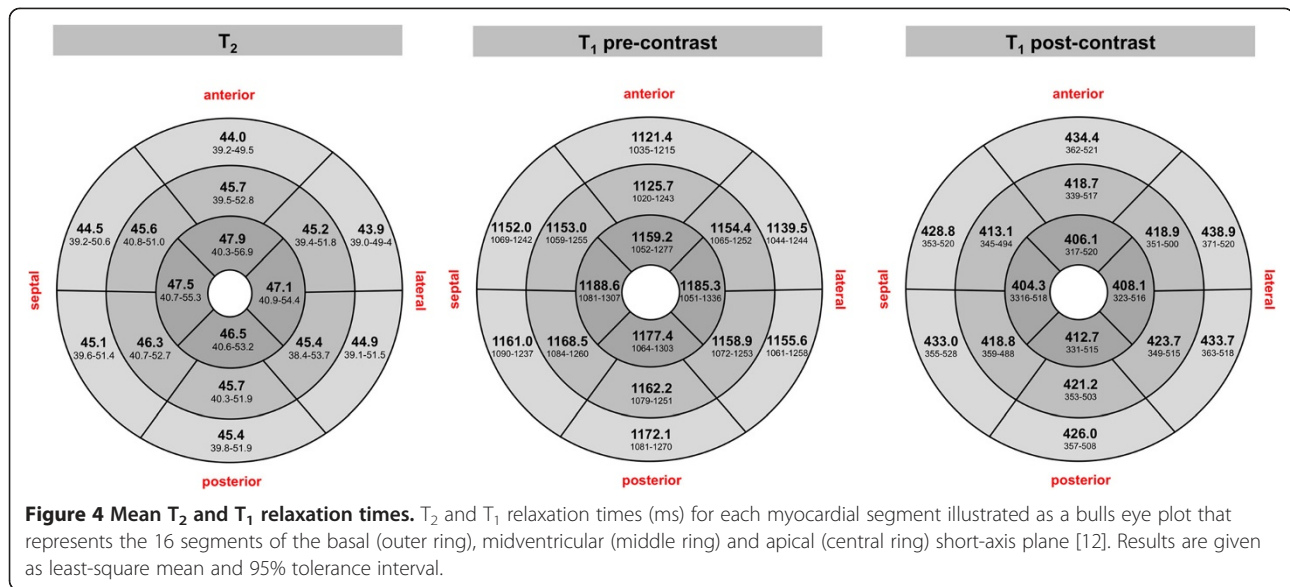

T_2 mapping

Previous studies with SSFP-based T_2 mapping at 1.5T did not report the exclusion of segments from analysis due to SSFP off-resonance or banding artifacts [2-4]. Hence, this challenge seems to surface at higher field strengths due to the increase in the peak-to-peak B_0 inhomogeneity across the heart. The use of an appropriately selected delta frequency may be an option to resolve some artifacts and deserves further systematic investigation. The artifacts mainly affected the inferolateral region, where pathologies like myocarditis may also exhibit their predominant lesion [13]. Despite that, the step from 1.5 T to 3 T for CMR is generally desired due to expected gains in signal, which may be exploited for improved spatial and temporal resolution. This potential promises to enable more detailed insights into cardiac tissue in order to facilitate the early detection of myocardial disease.

T_2 relaxation times derived from T_2 -prepared SSFP imaging in this study are higher compared to a black-blood multi-echo spin-echo approach at 3 T, which provided a mean value of $T_2 = 39.6$ ms in the septum [14]. Myocardial T_2 reported here was found to be lower versus a mean $T_2 = 52.2$ ms reported for T_2 prepared SSFP imaging at 1.5 T [2]. Possible explanations are: i) differences in the pulse sequence design, ii) differences in the spatial resolution, with lower resolution being associated with more partial volume and potentially higher T_2 values, and iii) T_1 relaxation effects due to higher T_1 values at 3 T versus 1.5 T. Generally, myocardial T_2 reported in the literature varies substantially, ranging from about 50 ms to 58 ms at 1.5 T [2]. The heterogeneity of data underlines that the measured T_2 relaxation time is very sensitive to cofactors and


emphasizes the need to generate reference values specific for each technique and imaging setting.

Our results showed that T_2 increased from base to apex, which is in accordance with a recent work using a similar mapping technique at 1.5 T [15]. The most probable cause is partial-volume effects that increase towards the apex owing to the curvature of the left ventricle. To encounter this limitation, some groups exclude the apical slice from mapping to omit measurement errors [6]. We tried to minimize this error by carefully drawing the contours in the middle of the myocardium while leaving out the endocardial portion of the myocardium, as well as by using an isotropic spatial resolution as high as possible.

Most of the previous studies reported T_2 values averaged over all myocardial segments or only for a midventricular slice. By averaging T_2 values over the whole slice or the whole heart, focal T_2 deviations may be overlooked. The present study is the largest study, which reports T_2 values for each myocardial segment and slice.

As reported for the global T_2 values, the segmental T_2 values increased from base to apex. In comparison, Markl et al. reported T_2 values from 50.5 ms to 51.6 ms in the basal slice and 54.3 ms to 56.1 ms in the apical slice at 1.5 T [15].

The inter-subject variability of absolute T_2 values was relatively large both per-slice and per-segment. This finding is in concordance with Thavendirathan et al., who described T_2 values ranging from about 50 ms to 62 ms in healthy controls [4], and with Giri et al., who reported that the apical region showed the most pronounced inter-subject variability [2]. The high inter-subject variability can be considered as the main challenge

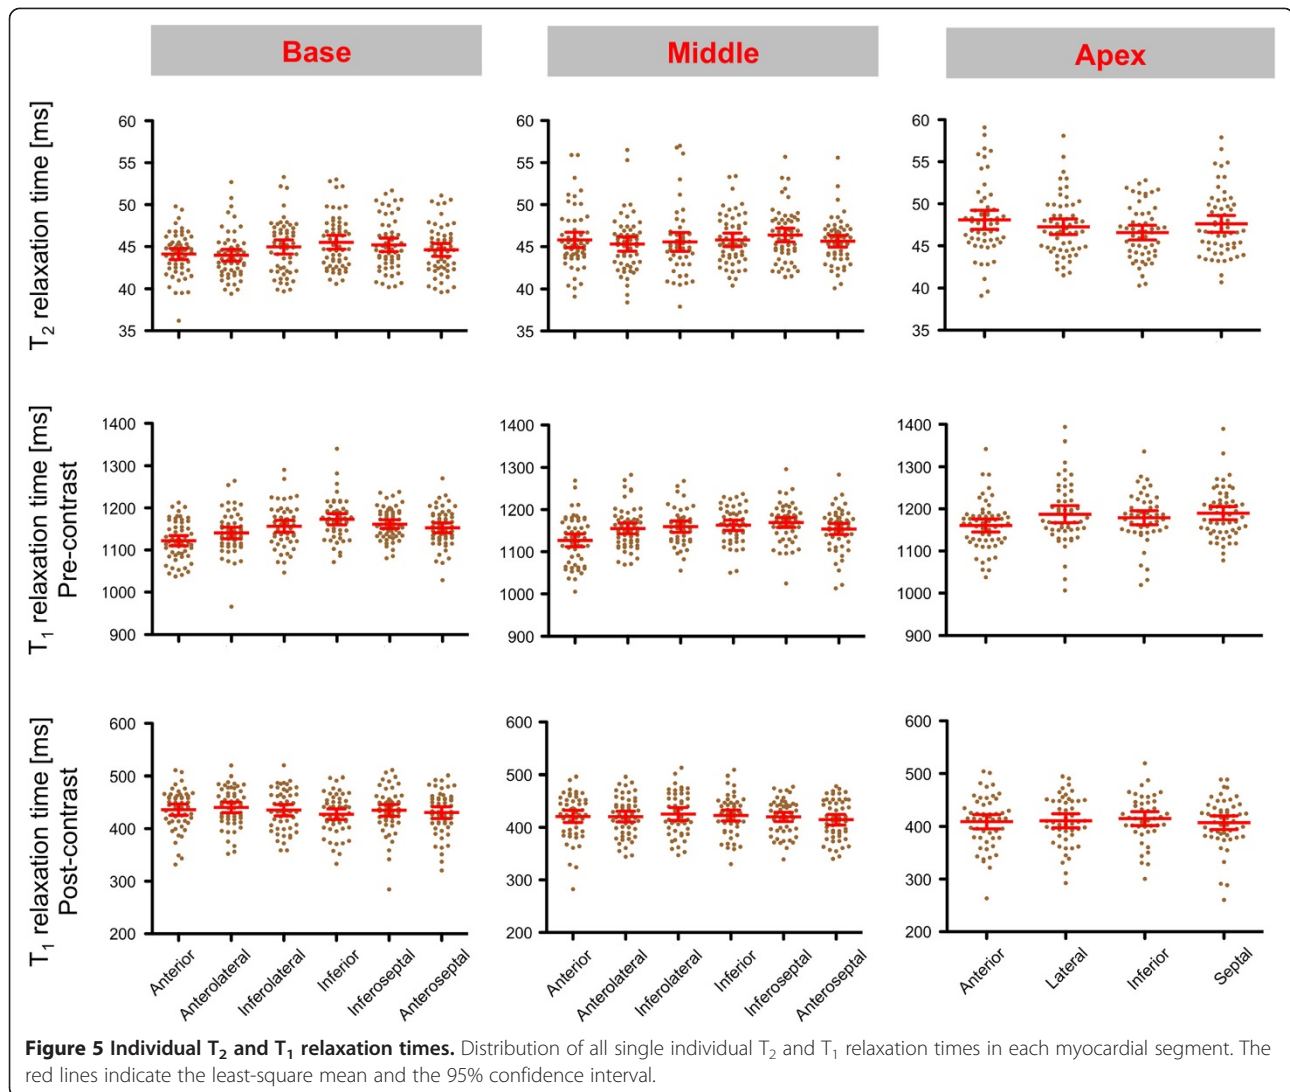

of T_2 mapping, given that the difference in T_2 between healthy and injured myocardium has been reported to be relatively small, e.g. 13 ms/11 ms between infarct core/myocarditis and remote myocardium [3,4].

The association of heart rate and T_2 relaxation time is under discussion. Giri et al. reported that the variability between healthy subjects was unrelated to heart rate. Other studies reported lower T_2 values in patients with higher heart rate [1,4]. This may be attributed to the hypothesis that higher heart rates induce pronounced T_1 relaxation effects caused by incomplete T_1 relaxation, which may affect T_2 mapping using a SSFP-based approach. This finding is very relevant for clinical practice as subtle T_2 increases may disappear in acutely ill patients with higher heart rates.

T_1 mapping

T_1 mapping demonstrated diagnostic image quality for the vast majority of myocardial segments. However, a

relevant number of myocardial segments had to be excluded due to technical challenges, which would lead to diagnostic uncertainty in a clinical scenario. Previous studies at 1.5 T and 3 T reported lower rates of artifact-related non-diagnostic segments [7,10,16,17]. The explicit source of the artifacts has not been reported in detail in most studies, which renders benchmarking against previous results challenging. A possible contributing factor might be that artifacts are often only visible in the original images - which are used for quality assessment - while they might be not apparent in the final maps. In our study, susceptibility artifacts in the inferolateral region were most frequent.

The pre-contrast T_1 values are in concordance with Piechnik et al., who reported $T_1 = 1169$ ms averaged over all myocardial segments [16]. At 3.0 T higher mid-ventricular T_1 values ($T_1 = 1315$ ms or $T_1 = 1286$ ms) were reported when using a T_1 mapping technique

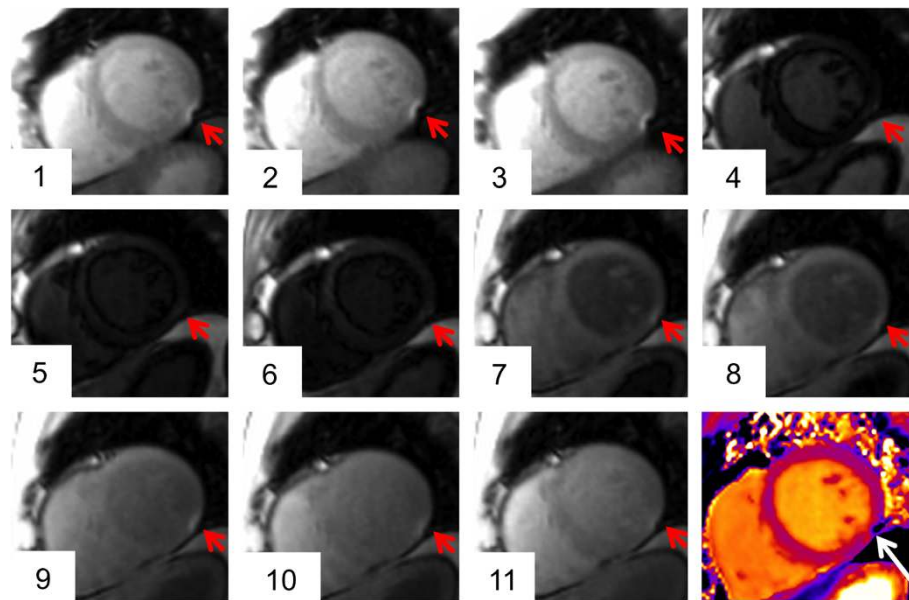


Figure 6 T₁ mapping artifact. Susceptibility artifact in the inferolateral wall of the midventricular plane (red arrow). The artifact was located at the border of the inferolateral and the inferior segment. In the corresponding map the artifact is hardly recognizable by visual assessment (white arrow).

similar to that used in this study [17,18]. These discrepancies underline that T₁ relaxation times are sensitive to many influencing factors.

The myocardial T₁ relaxation times reported here can be regarded as reference values specific only for this cohort, time point, mapping technique, type and dosage of contrast media. Further comparisons with other published results are difficult unless an identical study design is used. To provide a context, Lee et al. used 0.15 mmol Gadolinium DTPA and measured a mean T₁ of about 550 ms in one midventricular slice after 8.5 min in healthy human subjects at 3 T [17].

We observed that the pre-contrast T₁ times increased from base to apex, whereas the post-contrast T₁ values

decreased from base to apex. Partial-volume effects owing to the curvature of the left ventricle can most probably explain this finding with blood signal being included into the voxel. While some completely exclude apical T₁ maps from analysis [6], we tried to minimize this error by excluding the endocardial portion of the myocardium and by choosing a high isotropic spatial resolution.

In agreement with Kawel et al. we did not observe significant segment-to-segment differences post-contrast [7]. However, pre-contrast T₁ values of the anterior segments were lower than T₁ observed for the other segments. Interestingly, Piechnik et al. observed the identical pattern with MOLLI at 3 T [16]. Kawel et al.


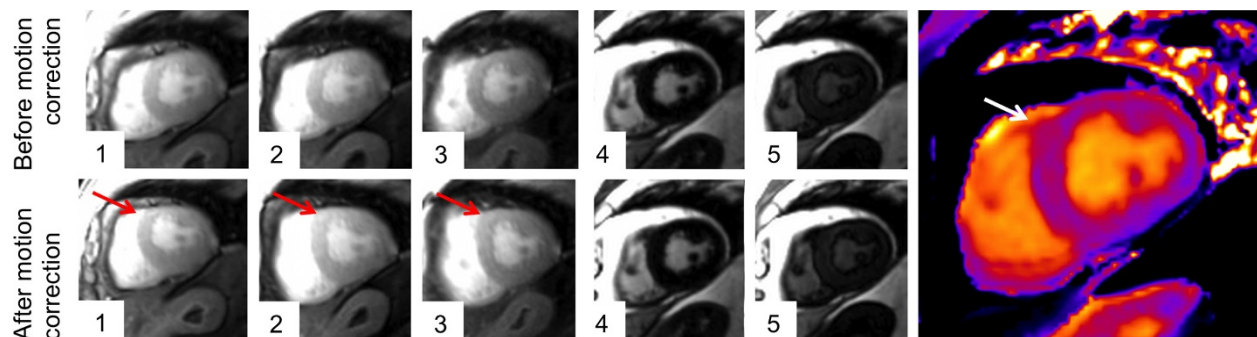


Figure 7 Failed motion correction during T₁ mapping. The original images (upper row) show the regular shape of the LV myocardium (the first five out of eleven images of the complete T₁ acquisition are depicted). The motion correction algorithm led to an outbound shift of the anterior and anteroseptal myocardial segment (red arrow in the bottom row). The corresponding map (right image) indicates an inhomogeneous T₁ distribution in this area (white arrow).

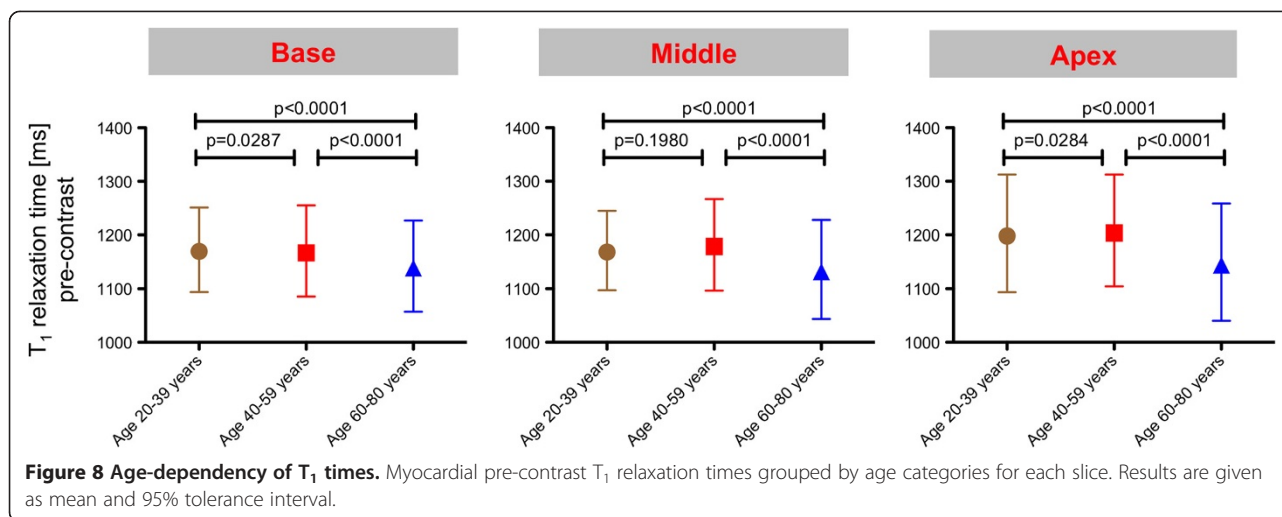

confirmed the presence of regional variability of pre-contrast T_1 values inspite of using a different classification into “septal” and “non-septal” myocardium [7]. Although absolute regional difference was small, this finding has to be considered in clinical CMR interpretation as the difference between healthy and abnormal tissue might be in a similar range.

The inter-subject variability of absolute T_1 values was notable both per-slice and per-segment, including extreme outliers. This finding is in concordance with other T_1 mapping studies reporting pre-contrast T_1 values at 1.5 T ranging from 862 ms to 1105 ms in healthy volunteers [19] and a coefficient of variation of 4.5% (pre-contrast) and 7.0% (post-contrast) [18]. The high inter-subject range may be the main challenge of T_1 mapping, given that the difference in T_1 times between healthy and injured myocardium has been reported to be relatively small depending on the underlying disease. Dall’Armellina et al. reported a mean pre-contrast T_1 value of 1257 ± 97 ms for acutely infarcted segments compared to 1196 ± 56 ms for normal unaffected segments at 3 T [20]. In other myocardial diseases like Fabry’s disease or amyloidosis, pre-contrast

T_1 may already be accurate enough to differentiate cardiac amyloid patients from normals [21].

Post-contrast T_1 in the present study was even more variable between subjects than pre-contrast T_1 , attributable to the many factors with influence on the contrast kinetics (e.g. patient weight, hematocrit, renal function). Miller et al. recently demonstrated that even though isolated post-contrast T_1 measurement showed significant within-subject correlation with histological collagen volume fraction, the between-subject correlations were not significant. Hence, isolated post-contrast T_1 measurement seems to be insufficient for assessing extracellular volume fraction [22].

Aging was found to be associated with decreasing pre-contrast T_1 values. This is an interesting aspect that may reflect early age-dependent alterations of myocardial texture. Dall’Armellina et al. and Ugander et al. showed that pre-contrast T_1 times were increased in acute myocardial ischemia [20,23]. Dass et al. reported increase in pre-contrast T_1 in cardiomyopathies. Hence, the present reduction of pre-contrast T_1 with age may sound contradictory [24]. In contrast, in a rat model, diffuse myocardial fibrosis was associated with a non-significant trend towards lower pre-contrast T_1 values [25]. Therefore our data are stimulating to further analyze the value of pre-contrast T_1 mapping in non-ischemic heart disease in future.

Table 3 Intra- and inter-observer dependency of the segmental quantification of T_2 and pre-contrast T_1 relaxation times

Technique	Correlation coefficient r	Bland-Altman: Bias \pm SD [ms]
T_2 – Intra-observer	0.95	0.0 ± 1.3
T_2 – Inter-observer	0.95	0.1 ± 1.1
T_1 – Intra-observer	0.93	4.6 ± 18.3
T_1 – Inter-observer	0.91	0.5 ± 20.2

Conclusion

In conclusion, myocardial T_2 and T_1 mapping at 3 T are feasible with a good diagnostic image quality, although susceptibility artifacts related to the magnetic field strength of 3 T triggered exclusion of myocardial segments from analysis. This study provides reference values for myocardial T_2 and T_1 relaxation times per slice and per segment for the specific MR setting, which were deduced from a large cohort of healthy volunteers.

With this approach a relatively high inter-subject distribution became apparent, which may constitute a relevant challenge for the definition of cut-offs that differentiate healthy from diseased myocardium in clinical practice.

Study limitations

i) As hematocrit was not measured in this study, its effect on T_2 and T_1 relaxation times could not be assessed. ii) Whereas observer variability to assess T_2 and T_1 relaxation times was low, the inter-scan variability was not assessed and deserves further investigation. iii) Regarding T_1 estimation by the applied MOLLI technique, there are known limitations to inversion efficiency [26] and to evaluation of magnitude based data. The inversion efficiency is also dependent on T_2 . At the time the study was designed, an improved inversion pulse designed for myocardial T_1 mapping tailored for myocardial T_2 was not available yet. The limitations of evaluating T_1 based on magnitude images are described in a recent publication [27]. By the time the study was designed, the proposed phase-sensitive recon was not yet available on our system.

Additional files

Additional file 1: T₂-mapping. A full set of T₂-weighted SSFP single shot images with 3 different T₂ preparation times and the corresponding T₂ maps from the basal, midventricular and apical slice.

Additional file 2: T₁-mapping. A full set of T₁-weighted SSFP single-shot images and the corresponding pre-contrast T₁ maps from the basal, midventricular and apical slice.

Competing interests

The co-author A. Greiser is employee of Siemens Healthcare, Germany. The other authors declare that they have no competing interests.

Authors' contributions

FvKB defined the design of the study, headed its coordination, acquired the image data, read the images, assisted in statistical analysis and drafted the manuscript. MP contributed to the analysis and interpretation of the data and was involved in drafting the manuscript. MD made contributions to acquisition of data and was involved in drafting the manuscript. RW and AG made substantial contributions to the analysis and interpretation of the data and were involved in drafting the manuscript. CS participated in the design of the study, performed the statistical analysis and was involved in drafting the manuscript. TN made substantial contributions to the acquisition, analysis and interpretation of the data and was involved in drafting the manuscript. JSM defined the design of the study, headed its coordination, assisted in statistical analysis and interpretation of the data, and drafted the manuscript. All authors read and approved the final manuscript.

Acknowledgements

The authors wish to acknowledge the technicians Kerstin Kretschel, Evelyn Polzin, Denise Kleindienst and Franziska Neumann for assisting in acquiring the CMR data, and the study nurses Elke Nickel-Szczzech and Antje Els for assisting in the organization of the CMR scans. This project was supported by a grant of the Else Kröner-Fresenius Stiftung (Bad Homburg, Germany).

Author details

¹Berlin Ultrahigh Field Facility, Max-Delbrueck Center for Molecular Medicine, Berlin, Germany. ²Working Group on Cardiovascular Magnetic Resonance, Experimental and Clinical Research Center a joint cooperation between the Charité Medical Faculty and the Max-Delbrueck Center for Molecular Medicine HELIOS Klinikum Berlin Buch, Department of Cardiology and Nephrology, Lindenberger Weg 80, 13125, Berlin, Germany. ³Siemens Healthcare, Erlangen, Germany. ⁴Scossis, Berlin, Germany. ⁵Experimental and Clinical Research Center, a joint cooperation between the Charité Medical Faculty and the Max-Delbrueck Center for Molecular Medicine, Berlin, Germany.

Received: 13 February 2013 Accepted: 3 June 2013

Published: 18 June 2013

References

1. Messroghli DR, Niendorf T, Schulz-Menger J, Dietz R, Friedrich MG. **T1 mapping in patients with acute myocardial infarction.** *J Cardiovasc Magn Reson.* 2003; **5**:353–9.
2. Giri S, Chung YC, Merchant A, Mihai G, Rajagopalan S, Raman SV, Simonetti OP. **T2 quantification for improved detection of myocardial edema.** *J Cardiovasc Magn Reson.* 2009; **11**:56.
3. Verhaert D, Thavendiranathan P, Giri S, Mihai G, Rajagopalan S, Simonetti OP, Raman SV. **Direct T2 quantification of myocardial edema in acute ischemic injury.** *JACC Cardiovasc Imaging.* 2011; **4**:269–78.
4. Thavendiranathan P, Walls M, Giri S, Verhaert D, Rajagopalan S, Moore S, Simonetti OP, Raman SV. **Improved detection of myocardial involvement in acute inflammatory cardiomyopathies using T2 mapping.** *Circ Cardiovasc Imaging.* 2012; **5**:102–10.
5. Flett AS, Hayward MP, Ashworth MT, Hansen MS, Taylor AM, Elliott PM, McGregor C, Moon JC. **Equilibrium contrast cardiovascular magnetic resonance for the measurement of diffuse myocardial fibrosis: preliminary validation in humans.** *Circulation.* 2010; **122**:138–44.
6. Wong TC, Piehler K, Meier CG, Testa SM, Klock AM, Aneizi AA, Shakesprere J, Kellman P, Shroff SG, Schwartzman DS, Mulukutla SR, Simon MA, Schelbert EB. **Association between extracellular matrix expansion quantified by cardiovascular magnetic resonance and short-term mortality.** *Circulation.* 2012; **126**:1206–16.
7. Kawel N, Nacif M, Zavodni A, Jones J, Liu S, Sibley CT, Bluemke DA. **T1 mapping of the myocardium: Intra-individual assessment of the effect of field strength, cardiac cycle and variation by myocardial region.** *J Cardiovasc Magn Reson.* 2012; **14**:27.
8. Xue H, Shah S, Greiser A, Guetter C, Littmann A, Jolly MP, Arai AE, Zuehlsdorff S, Guehring J, Kellman P. **Motion correction for myocardial T1 mapping using image registration with synthetic image estimation.** *Magn Reson Med.* 2012; **67**:1644–55.
9. MacFall JR, Riederer SJ, Wang HZ. **An analysis of noise propagation in computed T2, pseudodensity, and synthetic spin-echo images.** *MedPhys.* 1986; **13**:285–92.
10. Messroghli DR, Greiser A, Frohlich M, Dietz R, Schulz-Menger J. **Optimization and validation of a fully-integrated pulse sequence for modified look-locker inversion-recovery (MOLLI) T1 mapping of the heart.** *J Magn Reson Imaging.* 2007; **26**:1081–6.
11. Messroghli DR, Radjenovic A, Kozerke S, Higgins DM, Sivanathan MU, Ridgway JP. **Modified Look-Locker inversion recovery (MOLLI) for high-resolution T1 mapping of the heart.** *Magn Reson Med.* 2004; **52**:141–6.
12. Cerqueira MD, Weissman NJ, Dilsizian V, Jacobs AK, Kaul S, Laskey WK, Pennell DJ, Rumberger JA, Ryan T, Verani MS. **Standardized myocardial segmentation and nomenclature for tomographic imaging of the heart: a statement for healthcare professionals from the Cardiac Imaging Committee of the Council on Clinical Cardiology of the American Heart Association.** *Circulation.* 2002; **105**:539–42.
13. Abdel-Aty H, Boye P, Zagrosek A, Wassmuth R, Kumar A, Messroghli D, Bock P, Dietz R, Friedrich MG, Schulz-Menger J. **Diagnostic performance of cardiovascular magnetic resonance in patients with suspected acute myocarditis: comparison of different approaches.** *J Am Coll Cardiol.* 2005; **45**:1815–22.
14. Guo H, Au WY, Cheung JS, Kim D, Jensen JH, Khong PL, Chan Q, Chan KC, Tosti C, Tang H, Brown TR, Lam WW, Ha SY, Brittenham GM, Wu EX.

- Myocardial T2 quantitation in patients with iron overload at 3 Tesla. *J Magn Reson Imaging*. 2009; **30**:394–400.
15. Markl M, Rustogi R, Galizia M, Goyal A, Collins J, Usman A, Jung B, Foell D, Carr J. Myocardial T2-mapping and velocity mapping: Changes in regional left ventricular structure and function after heart transplantation. *Magn Res Med*. 2012. epub ahead of print.
 16. Piechnik SK, Ferreira VM, Dall'Armellina E, Cochlin LE, Greiser A, Neubauer S, Robson MD. Shortened Modified Look-Locker Inversion recovery (ShMOLL) for clinical myocardial T1-mapping at 1.5 and 3 T within a 9 heartbeat breathhold. *J Cardiovasc Magn Reson*. 2010; **12**:69.
 17. Lee JJ, Liu S, Nacif MS, Ugander M, Han J, Kawel N, Sibley CT, Kellman P, Arai AE, Bluemke DA. Myocardial T1 and extracellular volume fraction mapping at 3 tesla. *J Cardiovasc Magn Reson*. 2011; **13**:75.
 18. Kawel N, Nacif M, Zavodni A, Jones J, Liu S, Sibley CT, Bluemke DA. T1 mapping of the myocardium: intra-individual assessment of post-contrast T1 time evolution and extracellular volume fraction at 3T for Gd-DTPA and Gd-BOPTA. *J Cardiovasc Magn Reson*. 2012; **14**:26.
 19. Messroghli DR, Plein S, Higgins DM, Walters K, Jones TR, Ridgway JP, Sivananthan MU. Human myocardium: single-breath-hold MR T1 mapping with high spatial resolution–reproducibility study. *Radiology*. 2006; **238**:1004–12.
 20. Dall'Armellina E, Piechnik SK, Ferreira VM, Si QL, Robson MD, Francis JM, Cuculi F, Kharbanda RK, Banning AP, Choudhury RP, Karamitsos TD, Neubauer S. Cardiovascular magnetic resonance by non contrast T1-mapping allows assessment of severity of injury in acute myocardial infarction. *J Cardiovasc Magn Reson*. 2012; **14**:15.
 21. Karamitsos TD, Piechnik SK, Banyersad SM, Fontana M, Ntusi NB, Ferreira VM, Whelan CJ, Myerson SG, Robson MD, Hawkins PN, Neubauer S, Moon JC. Noncontrast t1 mapping for the diagnosis of cardiac amyloidosis. *JACC Cardiovasc Imaging*. 2013; **6**:488–97.
 22. Miller CA, Naish J, Bishop P, Coutts G, Clark D, Zhao S, Ray SG, Yonan N, Williams SG, Flett AS, Moon JC, Greiser A, Parker GJ, Schmitt M. Comprehensive validation of cardiovascular magnetic resonance techniques for the assessment of myocardial extracellular volume. *Circ Cardiovasc Imaging*. 2013; **6**:373–83.
 23. Ugander M, Bagi PS, Oki AJ, Chen B, Hsu LY, Aletras AH, Shah S, Greiser A, Kellman P, Arai AE. Myocardial edema as detected by pre-contrast T1 and T2 CMR delineates area at risk associated with acute myocardial infarction. *JACC Cardiovasc Imaging*. 2012; **5**:596–603.
 24. Dass S, Suttie JJ, Piechnik SK, Ferreira VM, Holloway CJ, Banerjee R, Mahmood M, Cochlin L, Karamitsos TD, Robson MD, Watkins H, Neubauer S. Myocardial tissue characterization using magnetic resonance noncontrast t1 mapping in hypertrophic and dilated cardiomyopathy. *Circ Cardiovasc Imaging*. 2012; **5**:726–33.
 25. Messroghli DR, Nordmeyer S, Dietrich T, Dirsch O, Kaschina E, Savwatis K, Oh-I D, Klein C, Berger F, Kuehne T. Assessment of diffuse myocardial fibrosis in rats using small-animal Look-Locker inversion recovery T1 mapping. *Circ Cardiovasc Imaging*. 2011; **4**:636–40.
 26. Kingsley PB, Ogg RJ, Reddick WE, Steen RG. Correction of errors caused by imperfect inversion pulses in MR imaging measurement of T1 relaxation times. *Magn Reson Imaging*. 1998; **16**:1049–55.
 27. Xue H, Greiser A, Zuehlsdorff S, Jolly MP, Guehring J, Arai AE, Kellman P. Phase-sensitive inversion recovery for myocardial T1 mapping with motion correction and parametric fitting. *Magn Reson Med*. 2013; **69**:1408–20.

doi:10.1186/1532-429X-15-53

Cite this article as: von Knobelsdorff-Brenkenhoff et al.: Myocardial T₁ and T₂ mapping at 3 T: reference values, influencing factors and implications. *Journal of Cardiovascular Magnetic Resonance* 2013 **15**:53.

Submit your next manuscript to BioMed Central and take full advantage of:

- Convenient online submission
- Thorough peer review
- No space constraints or color figure charges
- Immediate publication on acceptance
- Inclusion in PubMed, CAS, Scopus and Google Scholar
- Research which is freely available for redistribution

Submit your manuscript at
www.biomedcentral.com/submit

